

PRODUCT SPECIFICATION

Spec code: NOF-C0347
Product name: Semperguard® Nitrile Comfort
Date of issue: 29/08/14
Article number: 8167 8163.
= 3 (size S), 5 (size M), 7 (size L), 9 (size XL)

GENERAL INFORMATION

Type: single-use disposable examination or protective glove
Marking: all information on dispenser box
Shape: ambidextrous – straight fingers
Material: Nitrile Butadiene Rubber (NBR)
Colour: regular blue
Inner: online chlorinated/powder free
Outer: no treatment
Cuff/Surface: rolled cuff/finger textured

Thickness: (double measured)	Finger: min. 0.18 mm	Palm: min. 0.16 mm	Cuff: min. 0.10 mm
--	-----------------------------	---------------------------	---------------------------

Residual powder:	≤ 2 mg / glove
-------------------------	----------------

Force at break: [according to EN 455-2]	med. 6.0 N (during shelf life)
---	-----------------------------------

Length:	median 240 mm
----------------	---------------

Available Sizes:	S (6-7)	M (7-8)	L (8-9)	XL (9-10)
-------------------------	---------	---------	---------	-----------

Storage: 3 years storage life (date of expiration see on the box). Keep area cool, dry and dust free, avoid ventilation and storage close to photocopy equipment. Copper-ions discolour the glove. Protect gloves against ultraviolet light sources, as sunlight and oxidizing agents. Storage above 30°C will lead to accelerated aging and should be avoided.

STANDARDS, GUIDELINES AND QUALITY CERTIFICATION

Quality certification: ISO 9001, ISO 13485
Conformity to guidelines: Personal Protective Equipment 89/686/EEC: CE cat. III
Medical Device Directive 93/42/EEC: CE Class I

Conformity to standards:	EN 420	EN 374-2: specified	EN 374-3: Class 6
	EN 455	level 2 - AQL 1.5	Sodium Hydroxide 40%
	ASTM D6319	level 3: AQL <0.65 (G1)	
		level 2: AQL <1.5 (G1)	
		level 1: AQL <4.0 (S4)	

Conformity to food regulation: 1935/2004



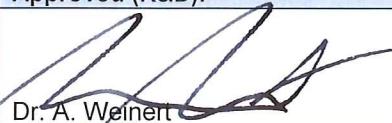


WARNING AND REPORTING SYSTEM

Potentially allergenic ingredients: Dithiocarbamate type, Zinc-mercaptobenzothiazol
(For further information, the actual version of the ingredients list is given on request.)

Medical Device Vigilance and Reporting System: According to the official reporting criteria of MDD, incidents caused by examination gloves or surgical gloves must be reported immediately to our medical device reporting officer. Tel.: +43 2630 310 ext. -510; Fax: -549

Caution! This product contains accelerators which may cause allergic reactions!

Established (PM):	Reviewed (QA):	Approved (R&D):
 L. Millonig, MA	 DI Dr. R. Stempfer, MSc	 Dr. A. Weinert